

1 THE MOLECULAR DETECTION FOR THE VIABILITY OF YERSINIA CELLS  
2 DURING SHOCK CHLORINATION – A PILOT SCALE STUDY  
3  
4  
5  
6  
7

8 P.S. Räsänen\*, J. Ikonen, A.-M. Hokajärvi and I.T. Miettinen  
9

10  
11 Water and Health unit, National Institute for Health and Welfare, P.O. Box 95, FI-70701  
12 Kuopio, FINLAND  
13

14 \* Corresponding author. Tel.: +358 29 524 6449; E-mail address: pia.rasanen@thl.fi  
15  
16  
17

18 1 INTRODUCTION  
19

20 Efficient decontamination of pipeline system is an essential action in situations where a  
21 drinking water distribution system is contaminated. The challenge in decontamination is  
22 the fact that biofilms may protect faecal and pathogenic microbes against disinfectant after  
23 contamination event.<sup>1,2</sup> The one of the most frequently used cleaning method for drinking  
24 water distribution networks is chlorination.<sup>3,4,5,6</sup> Shock-chlorination can be used for  
25 purification of microbial contaminated water distribution system in waterborne outbreaks.  
26 As an example, shock-chlorination was applied to clean the network after the severe  
27 waterborne outbreak in the Nokia city, Finland year 2007.<sup>5,7</sup>

28 It is also important to detect pathogenic microbes from water and biofilm samples as  
29 fast and efficient as possible if suspected contamination. The rapid and specific detection  
30 techniques for pathogenic bacteria could save valuable time and may reduce illness cases  
31 during an emergency situation. It also enables the verification of the success in the  
32 cleaning procedure.<sup>8</sup>

33 The new molecular biological techniques allow detection of viability of target  
34 pathogens as combination of Propidium monoazide (PMA)<sup>9</sup> treatment with quantitative  
35 polymerase chain reaction (qPCR) and Direct Viable Count (DVC) cell elongation with  
36 Peptide Nucleic Acid probes and Fluorescence in situ Hybridization (PNA-FISH).<sup>10</sup>  
37 Moreover, the traditional cultivation could take several days to weeks for reporting final  
38 results<sup>6</sup> when PCR and FISH based assays can provide results faster.<sup>8,11,12</sup> In addition, the  
39 FISH and PCR based techniques have been reported to be able to observe pathogenic  
40 bacteria from water and biofilm samples when the traditional cultivation method was not  
41 able to detect them.<sup>13, 8</sup>

42 The aim of this study was to test how a pilot water distribution network can be cleaned  
43 after contamination with bacteria using shock-chlorination.  
44  
45

46 2 THE EXPERIMENTAL SET-UP  
47


48 The pilot distribution system consisted of a 400m long PEX plastic pipeline. Water flow in  
49 the system was 1.8 l/min. The quality of water and growth of the biofilms was followed for  
50 a period of one month prior the contamination phase. The progress of decontamination was

1 followed with the chlorine concentration, DAPI staining and heterotrophic plate counts  
2 (HPC). The chlorine concentration used for shock-chlorination was 10 mg Cl<sub>2</sub>/l. During the  
3 experiment two parallel outlet water and three biofilm samples were taken in each sampling  
4 point.

5 The experiments were carried out using *Yersinia pseudotuberculosis* strain, the closest  
6 relative surrogate bacteria for severe human bacterial pathogen *Yersinia pestis*. The effect  
7 of shock-chlorination for microbiological agents was followed with new molecular biology  
8 techniques such as PMA-PCR and PNA-DVC-FISH assays for the determination of  
9 viability of the surrogate bacteria. A photoreactive PMA compound cannot pass through  
10 the cell membrane of a viable bacterial cell. When a cell membrane is damaged, the PMA  
11 gets into the cell and covalently binds to the cell genome. The attached PMA inhibits real-  
12 time PCR reactions which allow observing differences between viable and damaged  
13 cells.<sup>9,14</sup> The combination of DVC-FISH technique includes enrichment of samples in the  
14 presence of an antibiotic.<sup>10,15</sup> The antibiotic prevents normal cell division leading to  
15 elongation of viable cells.<sup>16</sup> A fluorescent PNA probe can bind as a sequence specific for  
16 ribosomal RNA of target cells. The successful binding between the PNA probe and  
17 specific target can microscopically be observed. When the fluorescent elongated cells  
18 could be detected the bacterial viability state can be estimated.<sup>17</sup> In addition, the *Yersinia*  
19 selective cefsulodin-Irgasan-novobiocin (CIN) plate counting was used as parallel with the  
20 new molecular biological techniques for detection of cultivable *Yersinia* cells.


### 21 22 23 3 RESULTS

24  
25 The concentration and viability of *Yersinia pseudotuberculosis* cells decreased rapidly in  
26 water and biofilm samples after start of the chlorination (Figure 1 and 2) as well as the  
27 counts of heterotrophic plate count and total microbial counts. In biofilms, the FISH counts  
28 of *Yersinia* were reduced by approximately 5 log and with qPCR 4 log.

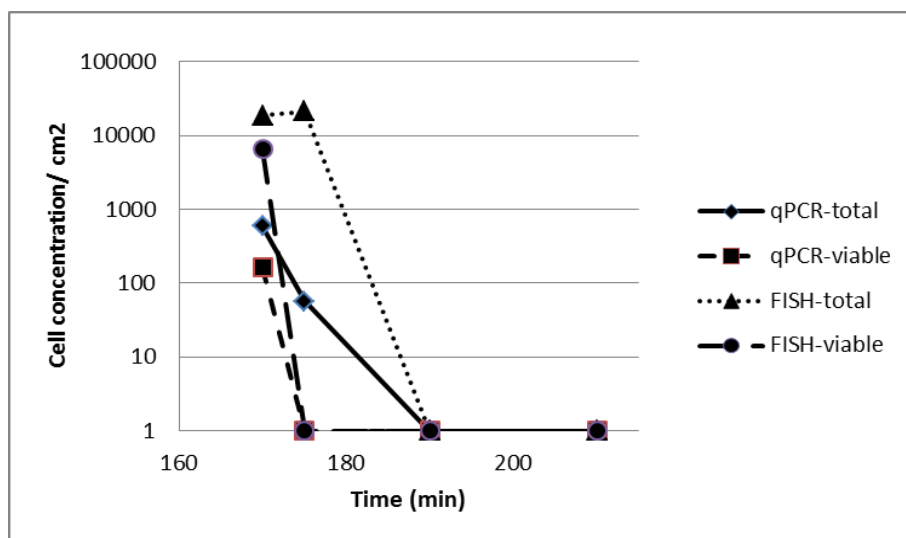

46 **Figure 1** The viable/ VBNC and total cell concentration in biofilm samples.  
47  
48  
49  
50

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50

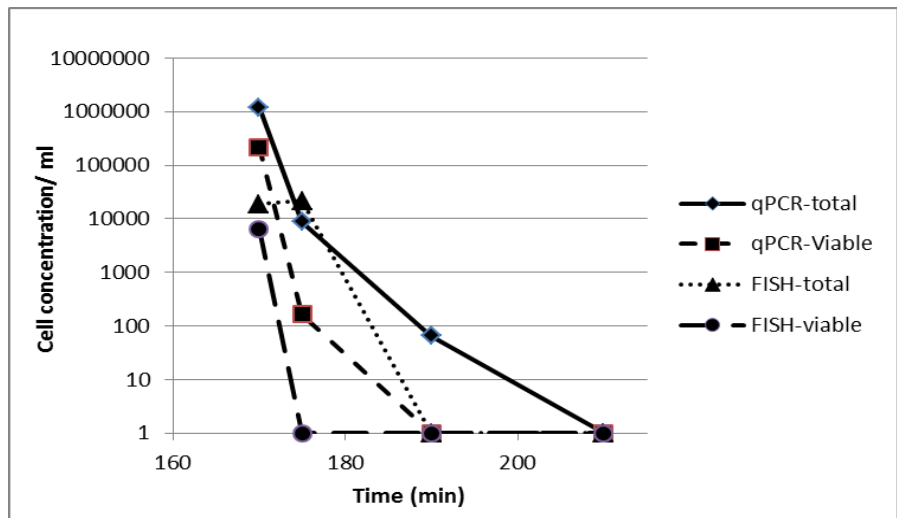

**Figure 2** The viable/ VBNC and total cell concentration in water samples.

In water, the FISH and qPCR counts of *Yersinia* were reduced by approximately 7 log. The new PCR and FISH techniques were able to detect *Yersinia* cells (total counts/ viable counts) while the selective culture method could not find any vegetative bacterial cells.

#### 4 CONCLUSIONS

In this study it was found out that the new qPCR and FISH based detection techniques were usable for determination of viability of the *Yersinia pseudotuberculosis* cells. According to previous studies, it has been stated that traditional FISH and PCR techniques could not separate live, viable but non-cultivable (VBNC) or dead cells from live culturable cells and that conventional cultivation based methods should be used for the detection of live, cultivable bacterial cells.<sup>6,18</sup> It is known that chlorine damages nucleic acids<sup>19</sup> which may affect the results of nucleic acid based FISH and qPCR methods. Overall, this study indicated that the shock-chlorination appeared to be an effective technique for cleaning a water distribution network after a bacterial contamination. However, it is obvious that some of the *Yersinia* cells introduced in the pipeline may have washed away from the pipeline network during the experiment. This might explain part of the rapid decrease in *Yersinia* cells in the water and biofilm samples. Therefore it is difficult to assess the true inactivation efficiency of shock-chlorination for the removal of the microbial contaminant.

#### Acknowledgements

This work has been done undertaken as part of a research project which is supported by the European Union within the Seventh Framework Programme (FP/2001-2011), Security Theme, “Increasing the security of citizens”, contract no 217976. There hereby follows a disclaimer stating that the authors are solely responsible for the work, it does not represent the opinion of the Community and the Community is not responsible for any use that might be made of data appearing herein.

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35

### References

- 1 U. Szewzyk, R. Szewzyk, W. Manz and K.H. Schleifer, *Annu. Rev. Microbiol.*, 2000, **54**, 81.
- 2 N. Trachoo, J.F. Frank and N.J. Stern, *J. Food Prot.*, 2002, **65**, 1110.
- 3 W.H. Farland and H.J. Gibb, 'U.S. perspective on balancing chemical and microbiological risks of disinfection' in *ILSI Press*, ed., G.C. Craun, Washington, D.C., 1993.
- 4 G.C. White, *Van Nostrand Reinhold Company Inc.*, New York, 1986.
- 5 O. Zacheus and I.T. Miettinen, *J. Water Health*, 2011, **9**, 763.
- 6 T. Pitkänen, J. Bräcker, I.T. Miettinen, A. Heitto, J. Pesola and E. Hakalehto, *Can. J. Microbiol.*, 2009, **55**, 849.
- 7 T. Pitkänen, I.T. Miettinen, U.-M. Nakari, J. Takkinen, K. Nieminen, A. Siitonen, M. Kuusi, A. Holopainen and M.-L. Hänninen, *J. Water Health*, 2008, **6**, 365.
- 8 R. Rimhanen-Finne, M.-H. Hänninen, R. Vuento, J. Laine, T.S. Jokiranta, M. Snellman, T. Pitkänen, I. Miettinen and M. Kuusi, *Scand. J. Infect. Dis.*, 2010, **42**, 613.
- 9 A. Nocker and A.K. Camper, *Appl. Environ. Microbiol.*, 2006, **72**, 1997.
- 10 J. Baudart and P. Lebaron, *J. Appl. Microbiol.*, 2010, **109**, 1253.
- 11 C. Almeida, N.F. Azevedo, R.M. Fernandes, C.W. Keevil and M.J. Vieira, *Appl. Environ. Microbiol.*, 2010, **76**, 4476.
- 12 S. Yang and R.E. Rothman, *Lancet Infect. Dis.*, 2004, **4**, 337.
- 13 M.J. Lehtola, T. Pitkänen, L. Miebach and I.T. Miettinen, *Water Sci. Technol.*, 2006, **54**, 57.
- 14 A. Nocker and A.K. Camper, *J. Microbiol. Methods*, 2006, **67**, 310.
- 15 T. Juhna, D. Birzniece, S. Larsson, D., Zulenkovz, A. Sharipo, N.F. Azevedo, F. Ménard-Szczebara, S. Castagnet, C. Féliers and C.W. Keevil, *Appl. Environ. Microbiol.*, 2007, **73**, 7456.
- 16 S. Larsson, L. Mezula and T. Juhna, *Techneau*, 2008.
- 17 L. Cerqueira, N.F. Azevedo, C. Almeida, T. Jardim, C.W. Keevil and M.J. Vieira, *Int. J. Mol. Sci.*, 2008, **9**, 1944.
- 18 J.E. Hobbie, R.J. Daley and S. Jasper, *Appl. Environ. Microbiol.*, 1977, **33**, 1225.
- 19 M.H. Phe, M. Dosset and J.C. Block, *Water Res.*, 2004, **38**, 3729.